

Quality is more than a word

ESPEC

Elevator type

# Thermal Shock Chamber

TSD-101-W

TSE-12-A



# Two-zone chamber capable of exposing specimens to a uniform thermal stress.

These two-zone thermal shock chambers are designed to specifically meet the needs of MIL, IEC, JASO and other international testing standards.


You can choose from 11L or 100L to fit your testing.

They come mounted with The N-instrumentation for improved operability and visibility, making remote monitoring and control via an Ethernet connection possible from your desk. Thermal shock chambers that apply uniform levels of thermal stress to specimens and that can be used in a wide range of fields, from research and development through to inspections and production.



## To minimize our chambers potential environmental impact

R-449A is the best alternative to R-404A

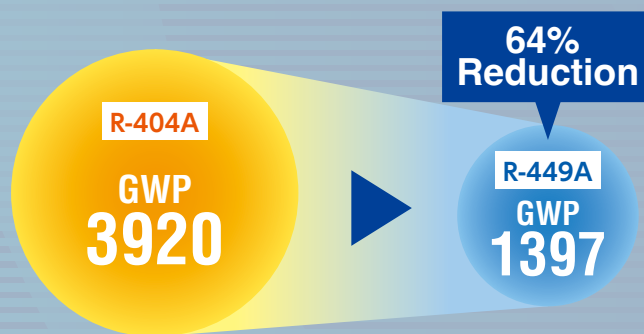

\*R-449A is available on request

11L



TSE-12-A

100L



TSD-101-W

\*The viewing window, casters (TSD) and recorder, emergency stop pushbutton (TSE) are optional.

# Features

## Reduce test time with a two-zone elevator type

| Model     |              | Volume | Test area        |
|-----------|--------------|--------|------------------|
| TSE-12-A  | Air-cooled   | 10.9L  | W320×H148×D230mm |
| TSD-101-W | Water-cooled | 100L   | W710×H345×D410mm |


### ● TSD specimen temperature recovery example (based on MIL-STD-883 Method 1010.9)

#### Test conditions

Hot exposure: +150°C for 30 min.  
Cold exposure: -65°C for 30 min.  
Specimens: ICs, 10 kg

#### Measurement conditions

Thermocouples were embedded in 10 ICs placed on two levels in each corner and in the center of a specimen basket.  
(Specimens embedded with thermocouples were placed beneath other ICs.)

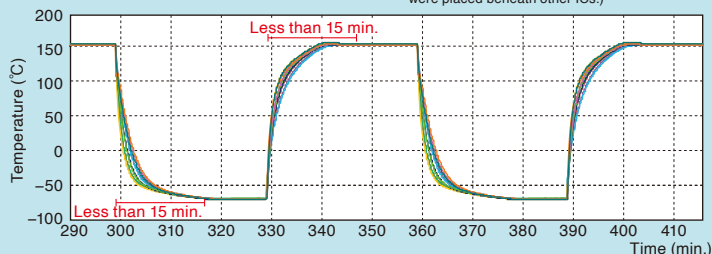


### ● TSD temperature uniformity example

#### Test conditions

Hot exposure: +150°C for 30 min.  
Cold exposure: -65°C for 30 min.  
Specimens: ICs (×10)

#### Measurement conditions

Thermocouples were attached to the surface of 10 ICs placed on two levels in each corner and in the center of a specimen basket.

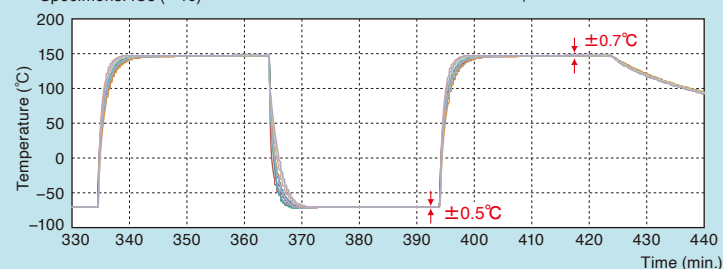

### ● Short temperature recovery time

### ● Meets international standards

Designed to comply with major environmental test standards such as IEC, JEDEC, EIAJ, MIL, JASO, IPC and SAE. (p.5 ~ 6)

### ● Transfer time within 10sec.

Test area transfer time between hot/cold chamber meets international test standards requirement.

### ● Improved temperature uniformity

Uniform airflow in the test area allows outstanding temperature uniformity. Uniform thermal stress is applied to each specimen, minimizing variation in test results.

### ● Smooth specimen transfer


“Soft move mode” is automatically activated when specimens move between the hot and cold chambers to reduce vibration and shock.



TSD



TSE

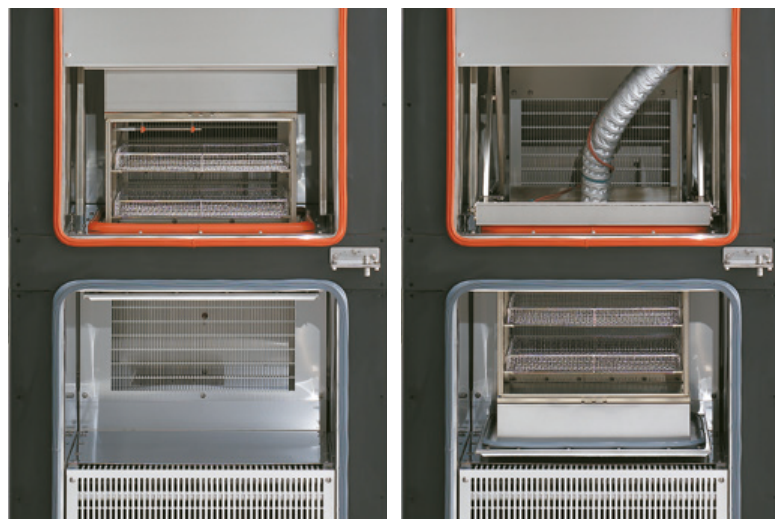

TSE hot exposure

TSE cold exposure

### ● Test area anti-drop mechanism to protect specimens

The test area's drive unit is equipped with a braking device to prevent specimens from falling the test area under any abnormal situations. For testing of small test samples, the specimen protective mesh which covered entire test area can be added. (Option)

# Features

## ● Easy wiring access

A cable port on right side allows for easy wiring for specimen measurement.



## ● Specimen Temperature Trigger (STT)

With up to two sensors attached to specimen(s), the STT function begins counting the exposure time once the specimen reaches a set temperature, or promptly activates moving of the specimen for the next exposure. This reduces overall testing time and ensures accurate specimen temperatures. Temperature readings can be recorded for each specimen and test area by connecting a temperature recorder. (TSD)



## ● Safe specimen handling thanks to ambient temperature recovery

The ambient temperature recovery feature intakes external air to return the test area to an ambient temperature after testing has finished or been paused. (TSD)

## ● Comprehensive safety system

A double safety system ensures that any transfer between test areas stops automatically when the door is open, and that the door locks while transfer is in progress.



TSD-101-W Specimen temperature measurement  
( Specimen temperature sensors Standard: 2 sensors  
Optional: additional 3 sensors )



TSD-101-W Test areas ( Top: hot chamber  
Bottom: cold chamber )



## TEST STANDARD AND COMPATIBLE MODELS

| Test standard                              |   | Temperature setting  |   | Soak time  | Recovery time   | Number of cycles                             | Model *    |
|--|---|--|---|--|---|--|------------|
|  |   | Hot (°C)   | Cold (°C)   |  |   |  |            |
| IEC 60068-2-14 Na<br>(JIS C 60068-2-14 Na) |   | +70 ± 2<br>+85 ± 2<br>+100 ± 2<br>+125 ± 2<br>+155 ± 2<br>+175 ± 2<br>+200 ± 2                   | -5 ± 3<br>-10 ± 3<br>-25 ± 3<br>-40 ± 3<br>-55 ± 3<br>-65 ± 3   | 3 hours<br>2 hours<br>1 hour<br>30 min.<br>10 min.<br>3 hours if not specified in product specifications                                       | 10% of soak time  | 5  | TSD<br>TSE |
| IEC 60749-25<br>(JESD22-A104F)             | A | +85 (+10, -0)  | -55 (+0, -10)   | 1/ 5/ 10/ 15 min.  | Specimen 5 to 14 min.                                     | Not specified                                | TSD        |
|  | B | +125 (+15, -0)   | -55 (+0, -10)   |  | Specimen 5 to 14 min.                                     |  |            |
|  | C | +150 (+15, -0)   | -65 (+0, -10)   |  | Specimen 5 to 29 min.                                     |  |            |
|  | H | +150 (+15, -0)   | -55 (+0, -10)   |  | Specimen 5 to 14 min.                                     |  |            |
|  | M | +150 (+15, -0)   | -40 (+0, -10)   |  | Specimen 5 to 15 min.                                     |  |            |
| IEC 61747-5 Na<br>(EIAJ ED-2531A Na)       |   | +100 ± 2<br>+95 ± 2<br>+90 ± 2<br>+85 ± 2<br>+80 ± 2<br>+75 ± 2<br>+70 ± 2<br>+65 ± 2<br>+60 ± 2 | -50 ± 3<br>-45 ± 3<br>-40 ± 3<br>-35 ± 3<br>-30 ± 3<br>-25 ± 3<br>-20 ± 3<br>-15 ± 3<br>-10 ± 3<br>-5 ± 3<br>-0 ± 3 | 3 hours<br>2 hours<br>1 hour<br>30 min.<br>10 min.<br>3 hours if not specified in product specifications                                       | 10% of soak time  | 5-10   | TSD<br>TSE |
| EIAJ ED-4701                               |   | Max. storage temp.   | Min. storage temp.  | 15g and below: at least 10 min.<br>15 to 150g: at least 30 min.<br>150 to 1,500g: at least 60 min.<br>More than 1,500g: individually specified | Air 5 min. or<br>10% of soak time,<br>whichever is longer | 10   | TSD        |
| EIAJ ED-4702                               | A | +125 (±3)  | -65 (±3)  | 30 min.  | Air 5 min. or<br>10% of soak time,<br>whichever is longer | 5 cycles<br>unless<br>otherwise<br>specified | TSD        |
|  | B | +100 (±3)  | -65 (±3)  |  |   |  |            |
|  | C | +100 (±3)  | -55 (±3)  |  |   |  |            |
|  | D | Mounted<br>printed circuit board<br>max. operating temp.   | Mounted<br>printed circuit board<br>min. operating temp.  |  |   |  |            |
| EIAJ ET-7407                               | A | +125 ± 5   | -25 ± 5   | 7 min. after specimen<br>temperature attainment  | —   | —  | TSD        |
|  | B | +125 ± 5   | -40 ± 5   |  |   |  |            |
|  | C | +80 ± 5  | -30 ± 5   |  |   |  |            |
|  | D | Max. operating<br>temp.  | Min. operating<br>temp.   |  |   |  |            |


## TEST STANDARD AND COMPATIBLE MODELS

| Test standard                |        | Temperature setting         |                 | Soak time  | Recovery time                    | Number of cycles | Model *    |
|------------------------------|--------|-----------------------------|-----------------|--|----------------------------------|------------------|------------|
|                              |        | Hot (°C)                    | Cold (°C)       |  |                                  |                  |            |
| MIL-STD-883<br>Method 1010.9 | A      | + 85(+ 10, − 0)             | − 55(+ 0, − 10) | 10 min. or longer<br>after transition start  | Specimen<br>less than<br>15 min. | At least 10      | TSD<br>TSE |
|                              | B      | + 125(+ 15, − 0)            | − 55(+ 0, − 10) |  |                                  |                  |            |
|                              | C      | + 150(+ 15, − 0)            | − 65(+ 0, − 10) |  |                                  |                  |            |
|                              | D      | + 200(+ 15, − 0)            | − 65(+ 0, − 10) |  |                                  |                  |            |
|                              | F      | + 175(+ 10, − 0)            | − 65(+ 0, − 10) |  |                                  |                  |            |
| JASO-D902                    | Type 1 | + 85                        | − 40            | Within 5 min. after solder<br>joint temp. reaches ±2°C of<br>preset temp. Or,<br>0.2kg and below: 0.5 hours<br>0.2 to 0.8kg: 1 hour<br>0.8 to 1.5kg: 1.5 hours<br>More than 1.5kg: 2 hours<br>preset temp. | Air 5 min.                       | 200              | TSD        |
|                              | Type 2 | Depends on parties involved |                 |  |                                  |                  |            |
| IPC-TM-650 2.6.6             | A      | + 125(+ 3, − 0)             | − 65(+ 0, − 5)  | 30 min.  | ————                             | 5                | TSD        |
|                              | B      | + 85(+ 3, − 0)              | − 55(+ 0, − 5)  |  |                                  |                  |            |
| SAE J1879                    |        | + 150                       | − 55            | 10 min. or longer<br>after transition start  | Specimen less than<br>15 min.    | 1000             | TSD        |

\* The test results may not meet specifications depending on the quantity of specimens or the setting method.


■ For further information, please contact us.

An easy-to-use, easy-to-read touch panel.

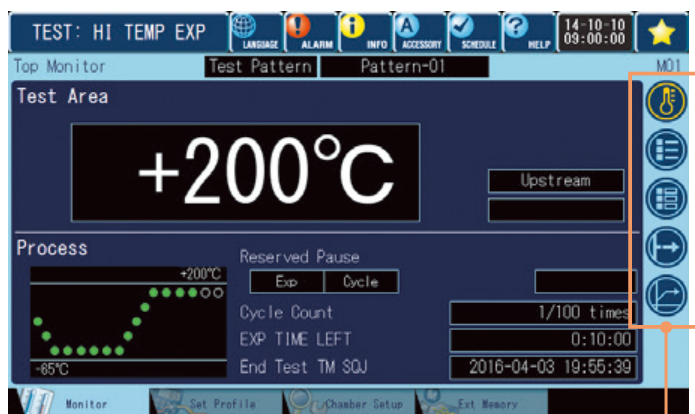

### Slide label

Touching an icon displays the menu label.

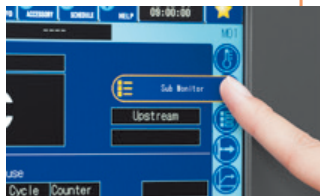

### Tabbed interface

High resolution 7-inch LCD. Tabs at the bottom make for quick and easy flipping between screens. Touching an icon displays the menu label which, touched, makes flipping between screens easier.


### Multilingual display

Use the language icon at the top of the display to change the display language from Japanese to English, Simplified Chinese, Traditional Chinese or Korean on any screen.

### Quick access button

For added convenience, the star (★) icon can have quick access functionality assigned, such as for jumping to a certain screen or directly launching a saved test pattern.

### Program copy and computer editing

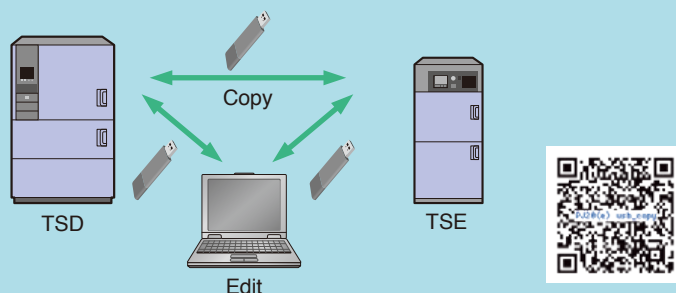

\* Some items may not be copied between different models and chambers with different options.

### Test data records

Temperature settings and measurements can be stored in the internal memory and exported with the use of USB flash drives. This enables them to be displayed as graphs on web browsers and stored for back-up purposes.

Test data can also be recorded in real time to a USB flash drive.

\* USB flash drives not included.

### Register up to 40 test patterns

### Download edit programs via online

The Pattern Manager Lite software installed on your PC, edit programs according to your testing needs, and upload them with a USB.



USB memory port

The Pattern Manager Lite software allows you to edit programs for your chamber, view and edit data as graph, etc. The software can be downloaded from the Test Navi website.



# Network

\* Requires an intranet

## Remote monitor and control (Ethernet connection)

The chamber comes with an ESPEC original web application. Connecting to the chamber Ethernet port (LAN's port) makes it possible to control chamber monitoring, pattern setting, operation start/stop, and other operations from a computer web browser. Installation of special software is not required. All you need is a standard computer web browser to connect with the chamber.

### Login privileges

| Screen Privileges | Chamber monitor | Pattern setting | Run/ Stop | Configuration |
|-------------------|-----------------|-----------------|-----------|---------------|
| Administrator     | ✓               | ✓               | ✓         | ✓             |
| Operator          | ✓               | ✓               | ✓         |               |
| User              | ✓               |                 |           |               |

## Edit test patterns on a web browser

Saved test programs can be edited on a web browser. Test programs can also be downloaded to your PC.

## E-mail alert

Alerts such as for a test ending, for maintenance, and errors are e-mailed to multiple recipients.

### Wireless LAN connection



#### Watch the videos


► Remote ON/OFF Operation




► Connecting Easily with Ethernet (LAN)



### Email alert

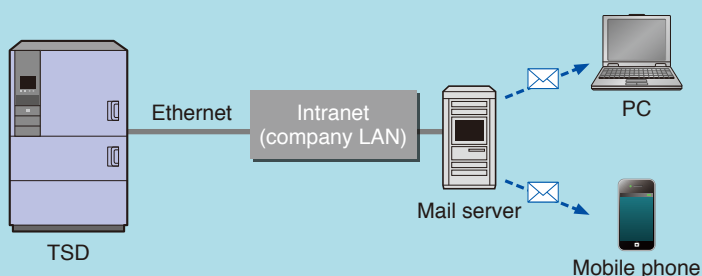

## ESPEC OnlineCore (Sold separately) Central control system recommended for multiple environmental test chambers installations

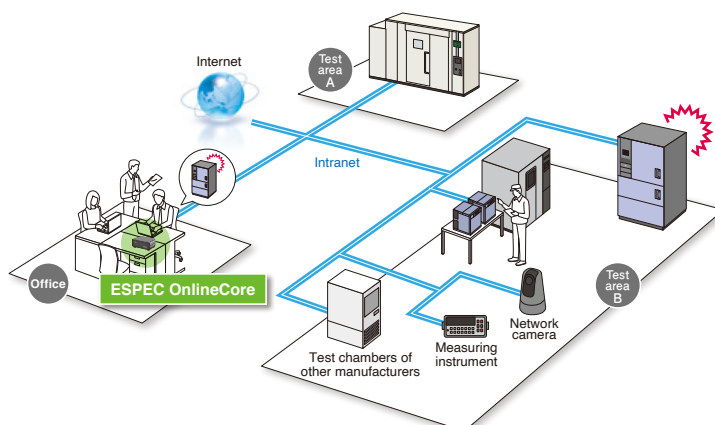

\*Please contact ESPEC for more information, about which products can be connected.

| Model                         |  |   | TSD-101-W  |                           |                        |                        |                               |
|-------------------------------|--|---|--|---------------------------|------------------------|------------------------|-------------------------------|
|                               |  |   | Water-cooled   |                           |                        |                        |                               |
| System                        |  |   | 2-zone transition by vertical transfer of specimens  |                           |                        |                        |                               |
| Performance *1                | Test area  | Hot exposure range  | + 60℃ to + 205℃  |                           |                        |                        |                               |
|                               |  | Cold exposure range   | − 77℃ to 0℃  |                           |                        |                        |                               |
|                               |  | Temp. fluctuation *2  | ± 1.0℃   |                           |                        |                        |                               |
|                               | Hot chamber                                      | Pre-heat upper limit  | + 205℃   |                           |                        |                        |                               |
|                               |  | Heat-up time *3   | Within 90 min from ambient temp. to + 200℃ (Setting: + 205℃)   |                           |                        |                        |                               |
|                               | Cold chamber                                     | Pre-cool lower limit  | − 77℃  |                           |                        |                        |                               |
|                               |  | Pull-down time *3   | Within 90 min from ambient temp. to − 77℃ (Setting: − 77℃)   |                           |                        |                        |                               |
|                               | Temp. recovery performance (2-zone)              | Recovery conditions   | • Hot exposure: + 150℃ (setting: + 155℃ 30 min)<br>• Cold exposure: − 65℃ (setting: − 68℃ 30 min)<br>• Sensor position: downstream<br>• Specimen: Plastic molded ICs, 10kg |                           |                        |                        |                               |
|                               |  | Temp. recovery time   | Specimen temp. within 15 min   |                           |                        |                        |                               |
|                               | Transfer time between hot & cold chambers        |   | Within 10 seconds  |                           |                        |                        |                               |
| Ambient recovery              | Recovery conditions                              | • Hot exposure: + 150℃ to max. + 55℃<br>• Ambient temp.: + 23℃<br>• Specimen: Plastic molded ICs, 10 kg |  |                           |                        |                        |                               |
|                               | Ambient temp. recovery time                      | Within 90 min   |  |                           |                        |                        |                               |
| Test area                     |  |   | Shelf brackets on 2 levels (up to 4 baskets can be installed)  |                           |                        |                        |                               |
| Refrigeration unit            | System   | Mechanical cascade refrigeration system   |  |                           |                        |                        |                               |
|                               | Compressor                                       | 3.73kW(5HP) scroll-type × 2   |  |                           |                        |                        |                               |
|                               | Refrigerant                                      | R-404A ( <a href="#">Low GWP Refrigerant</a> R-449A is available on request) , R-23                     |  |                           |                        |                        |                               |
| Cooler                        |  |   | Plate fin cooler and cold accumulator  |                           |                        |                        |                               |
| Elevating unit                |  |   | Power slider (250W)  |                           |                        |                        |                               |
| Inside dimensions             |  |   | W710×H345×D410 mm  |                           |                        |                        |                               |
| Test area capacity            |  |   | 100 L  |                           |                        |                        |                               |
| Load capacity of test area *4 |  |   | 30 kg  |                           |                        |                        |                               |
| Specimen basket load capacity |  |   | 5kg per basket   |                           |                        |                        |                               |
| Outside dimensions *5         |  |   | W1100×H1885×D1965 mm   |                           |                        |                        |                               |
| Weight                        |  |   | Approx. 1100 kg  |                           |                        |                        |                               |
| Utility requirements          | Ambient temp. range                              |   | + 5℃ to + 40℃  |                           |                        |                        |                               |
|                               | Power supply (Voltage fluctuation: rating ± 10%) |   | 200V AC<br>3 ϕ 3W 50/60Hz  | 208V AC<br>3 ϕ 3W 60Hz *6 | 220V AC<br>3 ϕ 3W 60Hz | 380V AC<br>3 ϕ 4W 50Hz | 400/415V AC<br>3 ϕ 4W 50Hz *7 |
|                               | Maximum load current                             |   | 64 A   | 62 A                      | 58 A                   | 34 A                   | 32 A                          |
|                               | Cooling water supply pressure *8                 |   | 0.2 Mpa Gauge to 0.5 Mpa Gauge (2 kg/cm² G to 5 kg/cm² G)  |                           |                        |                        |                               |
|                               | Cooling water supply rate *9                     |   | 2050L/ h (at reference water temp. + 25℃), 3400L/h (at reference water temp. + 32℃)  |                           |                        |                        |                               |
|                               | Piping connection size                           |   | Carbon steel pipe, ID 32 mm  |                           |                        |                        |                               |
|                               | Cooling water temp. range                        |   | + 5℃ to + 38℃  |                           |                        |                        |                               |
| Noise level *10               |  |   | Max. 65 dB   |                           |                        |                        |                               |
| Exhaust heat rate             |  |   | 12600 kJ/h (3000 kcal/h)   |                           |                        |                        |                               |
| Exhaust air volume            |  |   | 250 m³/h   |                           |                        |                        |                               |

<sup>\*1</sup> Under the conditions of a + 23°C ambient temperature, cooling water temperature + 25°C, rated voltage, and no specimen inside the test area.

<sup>\*2</sup> The performance values are based on IEC 60068-3-5:2001,

<sup>\*3</sup> When each chamber is operated independently

<sup>\*4</sup> When using the test area floor or heavy-duty shelves (option)

<sup>\*5</sup> Excluding protrusions


<sup>\*6</sup> This model complies with the requirements of the National Electric Code (NFPA 70) for the United States of America (NEC spec.)

<sup>\*7</sup> This model complies with the requirements of the European Community Directives (CE spec.)

<sup>\*8</sup> A pressure regulator valve is required if the pressure exceeds 0.5MPa Gauge (5kg/cm<sup>2</sup>G)

<sup>\*9</sup> Rate depends on the cleanliness of the heat exchanger

<sup>\*10</sup> Measurements are to be taken in an anechoic room at a height of 1.2m from the floor, and a distance of 1m from the front panel (ISO 1996-1: 2003.A-weighted sound pressure level)

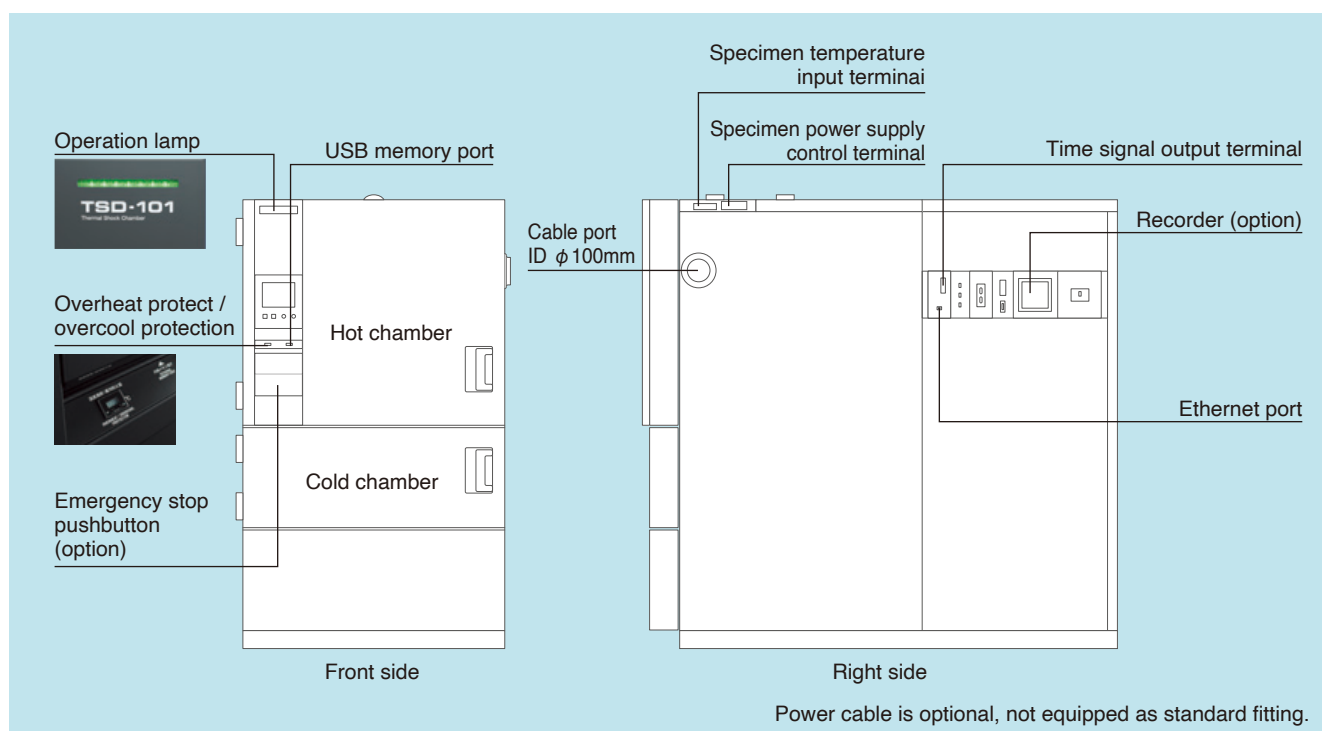


## SAFETY DEVICES

- Leakage breaker (200, 220V AC)
- Circuit breaker (208, 380, 400/415V AC)
- Electrical compartment door switch
- Hot chamber overheat protection switch
- Cold chamber overheat protection switch
- Hot chamber overheat protector (Built into temperature controller)
- Cold chamber overheat/ overcool protectors (Built into temperature controller)
- Test area overheat/ overcool protectors (Built into temperature controller)
- Test area overheat/ overcool protectors
- Circuit breaker
- Refrigerator high/ low pressure switch
- Compressor built-in protector
- Temperature switch for compressor
- Water suspension relay
- Temperature switch for air circulator
- Air circulator thermal relay
- Motor inverter
- Motor reverse prevention relay
- Hot chamber door switch
- Cold chamber door switch
- Door lock mechanisms
- Cartridge fuse
- Specimen power supply control terminal
- Cooling tower interlock terminal

## ACCESSORIES

- Specimen basket (18-8 Cr-Ni stainless steel: 5 mesh metal basket) W700 × H40 × D410 mm/ load capacity 5kg ..... 2

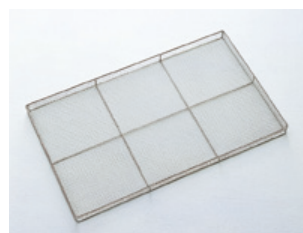

- Shelf brackets ..... 2 sets
- Cartridge fuse (3A, 5A, 7A, 10A, 15A) ..... 4
- Cable port rubber plug ..... 2
- Perforated cable port cap ..... 1
- Wire fisher (specimen wiring tool) ..... 1
- Thermocouple ..... 2
- Specimen temperature input connector ..... 2
- 3-pole socket (208V AC spec. only) ..... 3
- Nipple R1 1/4 in. (32 A) ..... 1
- Strainer R1 1/4 in. (32 A) ..... 1
- Strainer element R1 1/4 in. (32 A) ..... 1
- Breaker handle cover (except 208V AC) ..... 1
- Operation manual ..... 1
- Warranty card ..... 1

| Model                                     |  |                                       | TSE-12-A   |                        |                        |  |
|---|--|---------------------------------------|--|------------------------|------------------------|--|
|   |  |                                       | Air-cooled   |                        |                        |  |
| System                                    |  |                                       | 2-zone transition by vertical transfer of specimens  |                        |                        |  |
| Performance <sup>*1</sup>                 | Test area  | Hot exposure range                    | + 60℃ to + 200℃  |                        |                        |  |
|   |  | Cold exposure range                   | − 65℃ to 0℃  |                        |                        |  |
|   |  | Temperature fluctuation <sup>*2</sup> | ± 0.5℃   |                        |                        |  |
|   | Hot chamber                                      | Pre-heat upper limit                  | + 205℃   |                        |                        |  |
|   |  | Heat-up time <sup>*3</sup>            | Within 30 min. from ambient temp. to + 200℃ (Setting: + 205℃)  |                        |                        |  |
|   | Clod chamber                                     | Pre-cool lower limit                  | − 82℃  |                        |                        |  |
|   |  | Pull-down time <sup>*3</sup>          | Within 90 min. from ambient temp. to − 80℃ (Setting: − 82℃)  |                        |                        |  |
|   | Temp. recovery performance (2-zone)              | Recovery conditions                   | · Hot exposure: + 150℃, 30 min<br>· Cold exposure: − 65℃, 30 min<br>· Sensor position: Upstream<br>· Specimen: Plastic molded ICs 2 kg |                        |                        |  |
|   |  | Temp. recovery time                   | Within 5 min.  |                        |                        |  |
| Transfer time between hot & cold chambers |  |                                       | Within 10 seconds  |                        |                        |  |
| Construction                              | Test area  |                                       | Shelf brackets on 2 levels of fixed location   |                        |                        |  |
|   | Heater   |                                       | Stripped wire heater   |                        |                        |  |
|   | Refrigeration unit                               | System                                | Mechanical cascade refrigeration system  |                        |                        |  |
|   |  | Compressor                            | Rotary 1.5 kW × 2  |                        |                        |  |
|   |  | Refrigerant                           | R-404A ( <b>Low GWP Refrigerant</b> R-449A is available on request) , R-508A   |                        |                        |  |
|   | Cooler   |                                       | Plate fin cooler and cold accumulator  |                        |                        |  |
|   | Elevating unit                                   |                                       | Linear motor (55W)   |                        |                        |  |
| Test area capacity                        |  |                                       | W320 × H148 × D230mm   |                        |                        |  |
| Inner volume of test area                 |  |                                       | 10.9 L   |                        |                        |  |
| Load capacity of test area                |  |                                       | 8 kg   |                        |                        |  |
| Outside dimensions <sup>*4</sup>          |  |                                       | W680 × H1745 × D1050mm   |                        |                        |  |
| Weight                                    |  |                                       | Approx. 400kg  |                        |                        |  |
| Utility requirements                      | Ambient temp. range                              |                                       | 0 to + 40℃   |                        |                        |  |
|   | Power supply (Voltage fluctuation: rating ± 10%) |                                       | 200V AC<br>3 ϕ 3W 50/60Hz  | 220V AC<br>3 ϕ 3W 60Hz | 380V AC<br>3 ϕ 4W 50Hz | 400/415V AC<br>3 ϕ 4W 50Hz <sup>*5</sup> |
|   | Maximum load current                             |                                       | 26A  | 25A                    | 17A                    | 17A                                      |
| Noise level <sup>*6</sup>                 |  |                                       | Max.60dB   |                        |                        |  |
| Exhaust heat rate <sup>*7</sup>           |  |                                       | 17,585kJ/h (4200 kcal/h)   |                        |                        |  |

<sup>\*1</sup> The performance values are under the conditions of a +23°C ambient temperature, relative humidity of 65%rh, rated voltage, and no specimen. Heat up time and pull down time are those of single-unit operation of each chamber.

<sup>\*2</sup> The performance values are based on IEC60068-3-5:2001.


<sup>\*3</sup> Temperature heat-up/pull-down time account for performance of each temperature chamber.

<sup>\*4</sup> Excluding protrusions.

<sup>\*5</sup> Compliance with CE Marking.

<sup>\*6</sup> At 1m from front of chamber, 1.2m from floor. (ISO 1996-1:2003 A-weighted sound pressure level) depending on environment

<sup>\*7</sup> At ambient temperature +23°C.

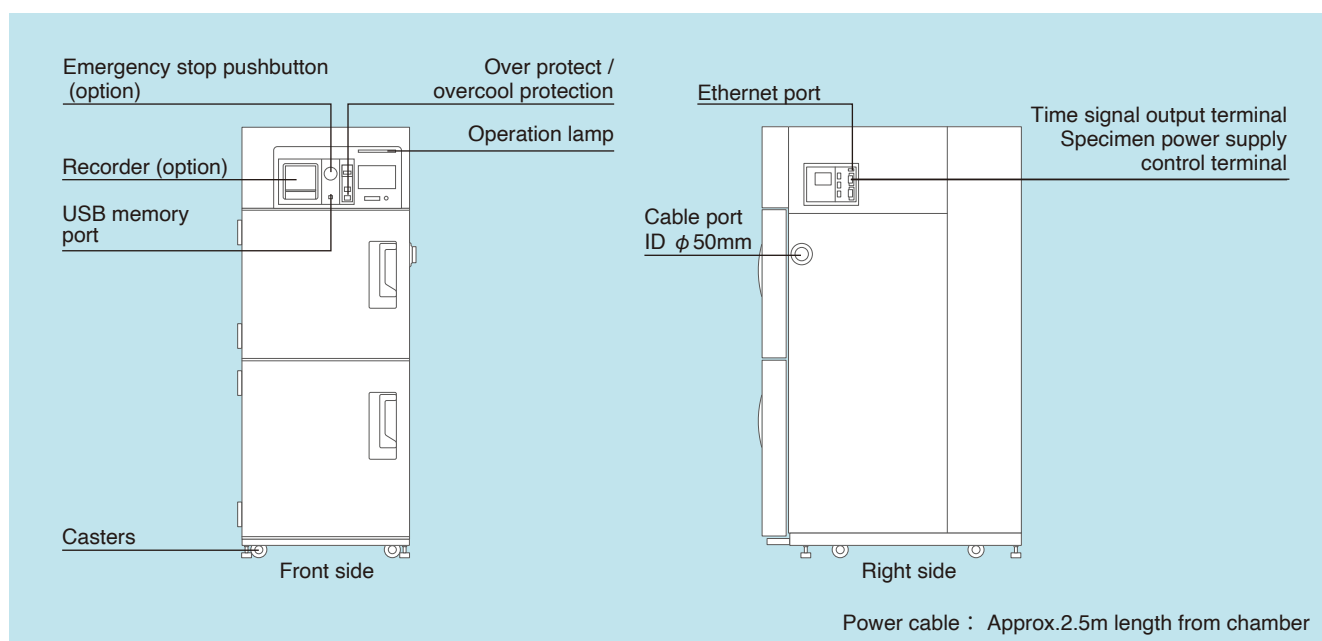

## SAFETY DEVICES

- Leakage breaker (200, 220V AC)
- Circuit breaker (380, 400 / 415V AC)
- Electrical compartment door switch
- Hot chamber overheat protection switch
- Cold chamber overheat protection switch
- Hot chamber overheat protector (Built into temperature controller)
- Cold chamber overheat / overcool protectors (Built into temperature controller)
- Test area overheat and overcool protectors (Built into temperature controller)
- Test area overheat / overcool protectors
- Refrigerator high pressure switch
- Thermal relay for compressor
- Temperature switch for compressor
- Temperature switch for air circulator
- Thermal relay for air circulator
- Motor inverter
- Motor reverse prevention relay
- Hot chamber door switch
- Cold chamber door switch
- Test area hold
- Door lock mechanisms
- Fuse
- Specimen power supply control terminal

## ACCESSORIES

- Specimen basket (18-8 Cr-Ni stainless steel, 5 mesh metal basket) W320×H35×D230mm /load capacity: 2kg ..... 2



- Cartridge fuse  
3A, 5A (200/220V AC) ..... 1each  
3A, 5A, 7A (380/400/415V AC) ..... 1each
- Cable port rubber plug ..... 2
- Wire fisher (specimen wiring tool) ..... 1
- Breaker handle stopper (200/220V AC only)
- Operation manual ..... 1
- Warranty card ..... 1



### Safety precautions

- Do not use specimens which are explosive or inflammable, or which contain such substances. To do so could be hazardous, as this may lead to fire or explosion.
- Do not place corrosive materials in the chamber. If corrosive substances or humidifying water is used, the life of the unit may be significantly shortened.
- Do not place life forms or substances that exceed allowable heat generation.
- Be sure to read the operation manual before operation.



## OPTIONS

## TSD-101-W / TSE-12-A

### Power cable

200V, 220V AC only

- 5 m
- 10 m

〈TSD〉

\* If this option is not specified, the chamber does not come with a power cable.

### Viewing window

TSD

Used for observation of the specimens inside the chamber.

Dimensions: W190 × H340 mm

Chamber lamp: Halogen lamp (× 1)



### Specimen basket/ shelf brackets

Equivalent to standard accessory.

Material: Stainless steel (5 mesh)

〈TSD〉

- Basket
- Shelf brackets

〈TSE〉

- Basket

### Heavy-duty shelf

TSD

Used to hold heavy specimen exceeding the load capacity of the standard specimen basket.

Load capacity: 15 kg

\* Equally distributed load, not included shelf brackets and specimen baskets.

### Additional cable port

TSD

Provided in addition to the standard cable port. (right side)

Location: Left side of the main unit

Internal diameter: 100 mm

### Cable port rubber plug

Prevents air leakage from the cable port.

### Interface

- RS-485C
- RS-232C
- GPIB

### Communication cables

- RS-485C 5m/10m/30m
- GPIB 2m/4m

### Temperature recorder (digital)

− 100°C to + 220°C /100 mm

- RK-61: 1 pen
- RK-63: 3 pens
- RK-64: 6 dots



### Paperless recorder

Records temperature of each section such as the temperature inside the chamber.

Display: 5.7inch color touch panel

Number of inputs (Initial setting):

- 1 (5 more channels can be turned ON)

Data saving cycle: 1 sec

- 3 (3 more channels can be turned ON)

Data saving cycle: 1 sec

- 3 (3 more channels can be turned ON)

Data saving cycle: 5 sec

- 5 (1 more channels can be turned ON)

Data saving cycle: 1 sec

- 5 (1 more channels can be turned ON)

Data saving cycle: 5 sec

- 6 Data saving cycle: 1 sec

- 6 Data saving cycle: 5 sec

Temperature range: − 100°C to + 220°C

Internal memory: 8MB

External memory media:

CF memory card (256 MB)

External memory function: USB port

Language support: ENG/ JPN

\* Select either built-in or portable type. (TSD)



### Recorder wiring

Preparation of a power cable, temperature sensor, and a grounding wire for additional installation in the future.

### Recorder terminal

Used to output the temperature within test area, hot chamber, cold chamber.

### Thermocouple

Attached to specimens to measure specimen temperature.

〈TSD〉

Thermocouple type T without ball  
(Copper/ Copper-Nickel)

〈TSE〉

T JIS C1602 with ball attached

- 2 m
- 4 m
- 6 m

### STT 3-point expansion

TSD

Additional 3 points of measuring the specimens' temperatures used for Specimen Temperature Trigger function.  
(2 points are equipped as standard.)

### Exposure signal output

TSD

A signal is output via a contact switch when test area temperature is within the user-selected range. This signal can be used to control peripheral instruments, like applying a voltage to specimens only during hot exposure, or monitoring test operation from a remote point.

### Total cycle counter

Indicates cycle counts.

Display range: 1-99999999

(with resetting function)



### Additional overhear protector

Additional preventive measures can be taken for excessive temperature rise in the chamber, in addition to the standard equipped double overhear protector.

### Emergency stop pushbutton

Stops the chamber immediately.



With cover



With guard



### Auxiliary cooling injector (LCO<sub>2</sub>)

Used to reduce the temperature recovery time of low temperature exposure by injecting liquefied carbon dioxide at beginning of exposure.


### Auxiliary cooling injector (LN<sub>2</sub>)

Used to reduce the temperature recovery time of low temperature exposure by injecting liquefied nitrogen at beginning of exposure.



### External alarm terminal

If the safety device of the chamber is activated, the external alarm terminal will notify it to a remote point.



TSD

### Anchoring fixtures

Used to bolt the chamber to the floor.

### Chamber dew tray

Prevents water leakage from the chamber onto the floor.

\* The use of casters is recommended to facilitate operation. (TSD)

\*To prevent damage in the event of water leakage, other preventive measures are also available.

### Casters

TSD

Installed for mobility.

Casters: 6

levelling-feet: 4



### Operation manual

- CD
- Booklet

### Reports & certificates

- Testing and inspection report
- Test data
- Calibration report
- Calibration certificate
- Traceability system chart
- Traceability certificate

**ESPEC CORP.** <https://www.espec.co.jp/english>

**Head Office**

3-5-6, Tenjinbashi, Kita-ku, Osaka 530-8550, Japan  
Tel: 81-6-6358-4741 Fax: 81-6-6358-5500

**ESPEC NORTH AMERICA, INC.**

Tel: 1-616-896-6100 Fax: 1-616-896-6150

**ESPEC EUROPE GmbH**

Tel: 49-211-361850-0

**ESPEC ENVIRONMENTAL CHAMBERS**

**SALES AND ENGINEERING LTD. STI. (Turkey)**

Tel: 90-212-438-1841 Fax: 90-212-438-1871

**ESPEC ENVIRONMENTAL EQUIPMENT (SHANGHAI) CO., LTD.**

**Head Office**

Tel: 86-21-51036677 Fax: 86-21-63372237

**BEIJING Branch**

Tel: 86-10-64627025 Fax: 86-10-64627036

**GUANGZHOU Branch**

Tel: 86-20-83317826 Fax: 86-20-83317825

**SHENZHEN Branch**

Tel: 86-755-83674422 Fax: 86-755-83674228

**SUZHOU Branch**

Tel: 86-512-68028890 Fax: 86-512-68028860

**TIANJIN Branch**

Tel: 86-22-26210366 Fax: 86-22-26282186

**XI'AN Branch**

Tel: 86-29-88312908 Fax: 86-29-88455957

**CHENGDU Branch**

Tel: 86-28-88457756 Fax: 86-28-88474456

**WUXI Branch**

Tel: 86-510-82735036 Fax: 86-510-82735039

**ESPEC TEST TECHNOLOGY (SHANGHAI) CO., LTD.**

Tel: 86-21-68798008 Fax: 86-21-68798088

**ESPEC ENGINEERING (THAILAND) CO., LTD.**

Tel: 66-3-810-9353 Fax: 66-3-810-9356

**ESPEC ENGINEERING VIETNAM CO., LTD.**

Mail : EEV\_support@espec-vn.com

**ISO 9001 (JIS Q 9001)**

**Quality Management System Assessed and Registered**

ESPEC CORP. has been assessed by and registered in the Quality Management System based on the International Standard ISO 9001:2015 (JIS Q 9001:2015) through the JSA Solutions Co.,Ltd.

\* The organization of these certificates is  
ESPEC CORP. Japan.



**ISO 27001 (JIS Q 27001)**

**Quality Management System Assessed and Registered**

\* The organization of these certificates is  
ESPEC CORP. Japan.



**ISO 14001 (JIS Q 14001)**

**Environmental Management System Assessed and Registered**

\* The organization of these certificates is  
ESPEC Group Japan.



●Specifications are subject to change without notice due to design improvements.

●Corporate names and trade names mentioned in this catalog are trademarks or registered trademarks.